Determination of ⁹⁹Mo contamination in ^{99m}Tc elute obtained from ⁹⁹Mo / ^{99m}Tc- generator

M. Momennezhad, S.R. Zakavi*, R. Sadeghi

Nuclear Medicine Research Center, Emam Reza Hospital, School of Medicine, Mashhad University of Medical Sciences, Mashhad, Iran

Background: 99mTc is a widely used radioisotope in nuclear medicine centers which is obtained by elution from Mo-99/Tc-99m generators. Usually the generators are either supplied by the Iran Atomic Energy Agency or by private companies from foreign countries. In this study we have measured 99Mo contamination in 99mTc elute from different generators in a period of one year. Materials and Methods: The radionuclide impurity of the 99mTc elute were studied in two types of radionuclide generators (A: produced in Iran and B: Imported from other country). In-vitro measurements were performed using dose calibrator. Direct measurements were made, using a standard canister at the time of milking of the generators and also in subsequent hours after milking. Results: The results showed a mean of 99Mo impurity in generators A and B to be 0.00932±0.0043 and 0.0170±0.0127 respectively. Although the results showed that the 99Mo contamination in 99mTc elute was lesser than the maximum accepted activity limit of 0.015%, the difference in these two types may reflect different methods of productions of generator, as well as the quality control procedures. Conclusion: The mean of 99Mo contamination in generators produced in Iran Atomic Energy Organization was lesser than generators imported from foreign origin. Iran. J. Radiat. Res., 2010; 8 (1): 31-35

Keywords: Nuclear generators, technetium, molybdenum contamination, dose calibrator.

INTRODUCTION

^{99m}Tc is a widely used radioisotope in nuclear medicine centers. This radionuclide is obtained from ⁹⁹Mo-^{99m}Tc generator by elution of generator with isotonic saline and should ideally contain no radionuclide impurity. However, due to imperfections in the production of the generator or possible occurrence of mechanical defects, ⁹⁹Mo may be eluted from the generator in the elution process ⁽¹⁻³⁾. The presence of ⁹⁹Mo in the eluted saline may interfere with labeling

process and decrease the labeling yield. Also, the radionuclide impurity introduces an unnecessary and unacceptable additional dose to the patients. The dose coefficient for ⁹⁹Mo is about 50 times higher than that of ^{99m}Tc ⁽²⁻⁴⁾. The high dose is associated with the beta particle and the higher energies of the photons emitted by 99Mo (4). Moreover, depending on the activity of the radionuclide impurity, the quality of the image can also be degraded (2). Figure 1 shows projections from myocardial perfusion scans, projections in upper three rows showed increased background activity and poor image quality as a result of Mo contamination. The lower three rows show projections from a myocardial perfusion scan with Tc-99m-MIBI uncontaminated with molybdinium.

Mostly ^{99m}Tc generators are supplied by AEOI and by a private company from foreign countries. In this study we have measured ⁹⁹Mo contamination in ^{99m}Tc elute from different generators during 1 year course.

MATERIALS AND METHODS

The radionuclide impurity of the ^{99m}Tc elute in two types (A & B) of radionuclide generators were studied. Fortyfour generators from Atomic Energy Organization of Iran (AEOI) [type A] and 25 generators from foreign country (Monrol, Turkey) [type B] were studied. The measurements were

*Corresponding author:

Dr. S. Rasoul Zakavi,

Nuclear Medicine Research Center, Emam Reza Hospital, School of Medicine, Mashhad University of Medical Sciences, Mashhad, Iran.

Fax: +98 511 8419521

E-mail: Zakavir@mums.ac.ir

accomplished during 1 year period and performed two times for each generator at the first day of shipment. The initial measurements were made just after milking and the second measurement was performed 3-5 hours after milking the generator on the same eluted vial, before labeling a new kit. In vitro measurements were made using dose calibrator. A Capintec CRC-15R calibrated dose calibrator (Capintec Inc. NJ, USA), with standard lead canister and insertion holder, was used to study the amount of 99Mo contamination (1). The procedure was as follows: At first the empty canister was measured at the Mo assay window to determine the background activity, then the elute of the sodium pertechnetate was measured inside the canister with the same window. The value showed the total amount of Mo and background and the net amount of Mo activity was determined after background subtraction (Mo - BG). To determine the activity of ^{99m}Tc, the elution was measured without the canister at the proper window (Tc). The ratio of Mo contamination was calculated by dividing the net Mo activity in μCi by the activity of Technetium (in mCi). The results were converted to MBq ⁹⁹Mo / MBq ^{99m}Tc by multiplying by 10⁻³. Univariate analysis was used for description of the variables and independent *t-test* was used for comparison of the quantitative data between groups.

SPSS software (version 11, SPSS Inc. USA) was used for the statistical analysis. P<0.05 was considered significant in all comparisons.

RESULTS

Table 1 shows the results of the ⁹⁹Mo contamination measured in 6 generators on the first day at the time of milking of the generators, and at subsequent hours to milking. The last two columns show the calculated ratio of contamination and the

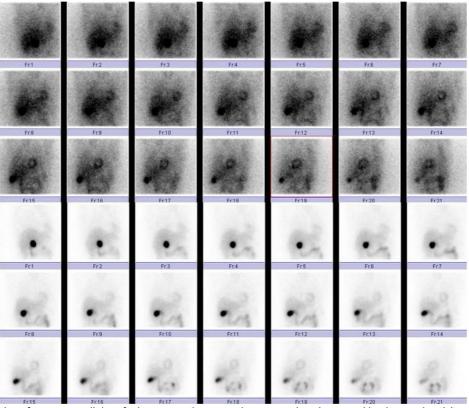


Figure 1. Projections from myocardial perfusion scans: the upper three rows show increased background activity and poor image quality as a result of Mo contamination compared to the normal state (lower three rows).

acceptable limit of 99Mo impurities, respectively.

Figure 2 shows the ratio of contamination measured in two types of generators compared to standard curve.

The results showed the mean of ⁹⁹Mo impurity in generators A and B were 0.00932±0.0043 and 0.0170±0.0127, respectively. Independent sample *t-test* showed that the mean of the ⁹⁹Mo impurity was significantly higher in group B of the generators.

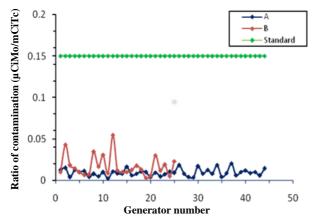


Figure 2. The ratio of ⁹⁹Mo contamination measured in generators A and B compared to acceptable amount.

DISCUSSION

The results of our study showed that the 99Mo contamination in 99mTc elute was lesser than the maximum accepted activity limit of 0.15 µCi of 99Mo per mCi of 99mTc in all generators. The mean of 99Mo contamination in generators produced by AEOI was lesser than imported generators which may be caused by different methods of production, possible mechanical damage in transportation and quality control procedures. It is important to note that whenever the generator is eluted, minimal amount of 99Mo is removed from the column; therefore, any eluted vial should be checked for 99Mo contamination. The amount of contamination can be estimated by direct measurement or in doubtful cases by means of energy checking and gamma spectrometry. When there is high contamination of ⁹⁹Mo in the solution, the spectrum can be investigated for high energy peaks in the range of 700-900 keV and the down scatters of ⁹⁹Mo can broaden the photopeak of ^{99m}Tc at 140 keV ⁽⁶⁾. Figure 3 shows the energy spectrums of 99mTc in normal condition (left) and in a high Mo contamination (right).

Table 1. Molybdenum contamination measured in 6 generators on the first day at the times of milking and at the subsequent hours after milking.

No	Generator	Milking Time	Reading Time	Tc (mCi)	Mo (uCi)	BG (uCi)	Mo-BG	Mo/Tc	Standard
1	A	8	8	284	3.8	2.6	1.2	0.004225	0.15
1	A		11	202	3.7	2.7	1	0.004950	0.15
2	A	8	8	283	3.7	2.6	1.1	0.003887	0.15
2	A		11	203	3.7	2.7	1	0.004926	0.15
3	A	8	8	190	3.9	2.6	1.3	0.006842	0.15
3	A		11	136	4	2.7	1.3	0.009559	0.15
4	В	8	8	1393	18	4.8	13.2	0.009476	0.15
4	В		11	785	15	4.2	10.8	0.013758	0.15
5	В	8	8	1188	55.3	4.11	51.19	0.043089	0.15
5	В		13	200	20.3	4.55	15.75	0.078750	0.15
6	В	8	8	849	37.1	8.12	28.98	0.034134	0.15
6	В		12.3	86.5	12.38	7.11	5.27	0.060925	0.15

The high energy peaks of the solution which has been due to 99Mo contamination are shown in figure 4. This spectrum was obtained by multi channel analyzer and a scintillation probe.

A similar study has shown that the Mo contamination in one generator was more than ten times of impurity activity limit of 0.015% in the ^{99m}Tc elutes ⁽³⁾. According to our knowledge, no other study was found in the literature regarding comparison of different generators in a large scale.

The presence of Mo contamination in the body can be confirmed using other in vitro techniques, and direct in vivo measurements, while more time is required by these methods (2, 4).

In conclusion this study indicated the importance of performing quality control procedures in nuclear medicine centers. especially on the radionuclide generators. Every Tc-99m elute should be tested for radionuclide purity and any vial with unacceptable Mo-99 contamination must be discarded. The Molybdenum break through (MBT) must be determined at least for the first elution of each generator (7, 8).

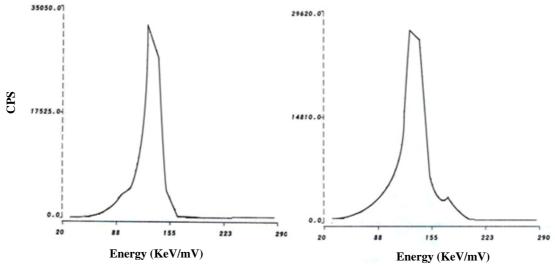


Figure 3. The photopeak of 99mTc recorded by a gamma camera with no 99Mo contamination (Left) versus high 99Mo contamination (Right). Note the widening of the peak on the right.

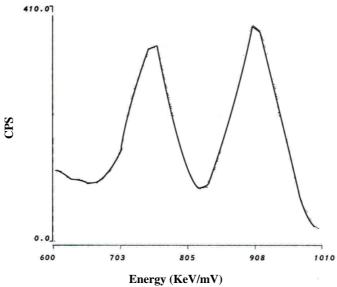


Figure 4. The high energy photopeak of Pertechnetate solution due to 99Mo contamination.

REFERENCES

- Williams CC, Kereiakes JG, Grossman LW (1981) The accuracy of 99Molybdenum assays in 99mTechnetium solutions. Radiology, 138: 445-8.
- Da. Silva C, Riberio BS, Souza WO, Araujo F, Kucena EA, Dantas ALA, Dontas BM (2007) Application of bioassay techniques to evaluate ⁹⁹Mo incorporation in nuclear medicine patients. International Nuclear Atlantic Conference - INAC 2007 Santos, SP, Brazil, September 30 to October 5, 2007.
- 3. Fatima N, Zaman M, Niayz K, Raza H, Iqbal J, Hameed A, Hashmi H, Habib S (2008) Effective method to minimize molybdenum content of 99 molybdenum-99mTechnetium generator eluate. *Pakistan Journal of Radiology (PJR)*, **18**: 20-21.
- Maranhão Dantas B, Almeida Dantas A, Navarro Marques F, Bertelli L and Stabin MG (2005)

- Determination of ⁹⁹Mo contamination in a nuclear medicine patient submitted to a diagnostic procedure with ⁹⁹mTc. *Braz Arch Biol Technol*, **48**:215-220.
- Urbano N, Modoni S, Guerra M and Chinol M (2005) Evaluation of fresh and old eluate of ⁹⁹Mo/^{99m}Tc generators used for labeling of different pharmaceutical kits. J Radioanal Nucl Chem, 265: 7-10.
- Vucina JL (1996) Radionuclide purity of 99mTC eluate for use in nuclear medicine. Med Pregl, 49: 41-4.
- Chianta M (2008) Covidien imaging solutions potential for molybdenum-99 breakthrough: http:// www.aapm.org/government_affairs/Covidien.asp Date of access: 29/June/2009.
- Reese IC and Mishkin FS (1968) A simple method of reducing the molybdenum content of the eluate from a 99Mo-Tc99m generator. Am J Roentgenol Radium Ther Nucl Med, 103: 896.